

**TSH Receptor Autoantibody  
2<sup>nd</sup> Generation ELISA Kit -  
Instructions for use**



**RSR Limited**

Parc Ty Glas, Llanishen,  
Cardiff CF14 5DU United Kingdom  
Tel.: +44 29 2068 9299 Fax: +44 29 2075 7770  
Email: [info@rsrltd.com](mailto:info@rsrltd.com) Website: [www.rsrltd.com](http://www.rsrltd.com)

**EC REP** Advena Ltd. Tower Business Centre, 2<sup>nd</sup> Flr.,  
Tower Street, Swatar, BKR 4013 Malta.

**INTENDED USE**

The RSR TSH receptor (TSHR) autoantibody (TRAb) ELISA kit is intended for use by professional persons only for the quantitative determination of TRAb in human serum. Hyperthyroidism in Graves' disease is due to the presence of autoantibodies to the TSHR and measurement of these autoantibodies can be useful in disease diagnosis and management.

**REFERENCES**

J. Bolton et al  
Measurement of thyroid stimulating hormone receptor autoantibodies by ELISA  
Clin. Chem. 1999 45: 2285-2287

K. Kamijo  
TSH receptor antibody measurement in patients with various thyrotoxicosis and Hashimoto's thyroiditis: a comparison of two two-step assays, coated plate ELISA using porcine TSH receptor and coated tube radioassay using human recombinant TSH receptor  
Endocrine Journal 2003 50:113-116

B. Rees Smith et al  
A new assay for thyrotropin receptor autoantibodies  
Thyroid 2004 14: 830-835

**ASSAY PRINCIPLE**












In RSR's TRAb ELISA, TRAb in patients' sera, calibrators and controls are allowed to interact with TSHR coated onto ELISA plate wells. After a 2 hour incubation, the samples are discarded leaving TRAb bound to the immobilised TSHR. TSH-Biotin is added in a 2<sup>nd</sup> incubation step, where it interacts with immobilised TSHR which have not been blocked by the bound TRAb from patient sera, calibrators or controls. The amount of TSH-Biotin bound to the plate is then determined in a 3<sup>rd</sup> incubation step by addition of Streptavidin Peroxidase (SA-POD), which binds specifically to Biotin. Excess unbound SA-POD is then discarded and the addition of the peroxidase substrate 3,3',5,5'-tetramethylbenzidine (TMB) results in the formation of a blue colour. This reaction is stopped by the addition of stop solution causing the well contents to turn from blue to yellow. The absorbance of the yellow reaction mixture at 450nm is then read using an ELISA plate reader. A lower absorbance indicates the presence

of TRAb in a test sample as TRAb inhibits the binding of TSH-Biotin to TSHR coated plate wells. The measuring range is 1 – 40 IU/L (NIBSC 08/204).

**STORAGE AND PREPARATION OF TEST SERUM SAMPLES**

Sera to be analysed should be assayed soon after separation or stored, preferably in aliquots, at or below –20°C. 150 µL is sufficient for one assay (duplicate 75 µL determinations). Repeated freeze thawing or increases in storage temperature must be avoided. Incorrect storage of serum samples can lead to loss of TRAb activity. Do not use lipaemic or haemolysed serum samples. Do not use plasma in the assay. When required, bring test sera to room temperature (20 – 25°C) and mix gently to ensure homogeneity. Centrifuge the serum prior to assay (preferably for 5 minutes at 10-15,000 rpm in a microfuge) to remove any particulate matter. Please do not omit this centrifugation step for sera that are cloudy or contain particulates.

**IFU SYMBOLS**

Symbol	Meaning
	EC Declaration of Conformity
	In Vitro Diagnostic Device
	Catalogue Number
	Lot Number
	Consult Instructions
	Manufactured by
	Sufficient for
	Expiry Date
	Store
	Negative Control
	Positive Control

**MATERIALS REQUIRED AND NOT SUPPLIED**

Pipettes capable of dispensing 50 µL, 75 µL and 100µL.

Means of measuring out various volumes to reconstitute or dilute reagents.

Pure water.

ELISA Plate reader suitable for 96 well formats and capable of measuring at 450nm.

ELISA Plate shaker, capable of 500 shakes/min (not an orbital shaker).

ELISA Plate cover.

## PREPARATION OF REAGENTS SUPPLIED

Store unopened kits and all kit components (A-K) at 2–8°C.

A	<b>TSH Receptor Coated Wells</b> 12 breakapart strips of 8 wells (96 in total) in a frame and sealed in a foil bag. Allow to stand at room temperature (20-25°C) for at least 30 minutes before opening.
	Ensure wells are fitted firmly into frame provided. After opening, return any unused wells to the original foil bag and seal, then place the foil bag in the self-seal plastic bag with desiccant provided. Store at 2-8°C for up to expiry of kit.
B	<b>Start Buffer</b> 10 mL Ready for use
C1-4	<b>Calibrators</b> 1, 2, 8 and 40 IU/L (units are NIBSC 08/204) 4 x 1.0 mL Ready for use
D1	<b>Negative Control</b> 1.0 mL Ready for use
D2	<b>Positive Control (See label for range)</b> 1.0 mL Ready for use
E	<b>TSH-Biotin</b> 3 vials Lyophilised
	Reconstitute each vial with 4.5 mL reconstitution buffer for TSH-Biotin (F). When more than one vial is to be used, pool the vials and mix gently before use. Store at 2–8°C for up to expiry of kit.
F	<b>Reconstitution Buffer for TSH-Biotin</b> 15 mL Ready for use
G	<b>Streptavidin Peroxidase (SA-POD)</b> 0.75 mL Concentrated
	Dilute 1 in 20 with diluent for SA-POD (H). For example, 0.5 mL (G) + 9.5 mL (H). Store at 2–8°C for up to expiry of kit.
H	<b>Diluent for SA-POD</b> 15 mL Ready for use
I	<b>Peroxidase Substrate (TMB)</b> 15 mL Ready for use
J	<b>Concentrated Wash Solution</b> 100 mL Concentrated
	Dilute to 1 litre with pure water before use. Store at 2–8°C for up to expiry of kit.
K	<b>Stop Solution</b> 10 mL Ready for use

## ASSAY PROCEDURE

Allow all reagents and test samples to stand at room temperature (20-25°C) for at least 30 minutes before use. A repeating Eppendorf type pipette is recommended for steps 1, 5, 8, 10 and 11. Duplicate determinations are strongly recommended for test sera, calibrators and controls.

1.	Pipette <b>75 µL</b> of start buffer (B) into each well to be used, leaving the last well empty for a blank (see step 12).
2.	Pipette <b>75 µL</b> of test sera, calibrators (C1-4) and controls (D1 and D2) into respective wells (start with the 40 IU/L calibrator and descend down the plate to the negative control and then test sera, in duplicate is recommended), leaving the last well blank.
3.	Cover the frame and shake the wells for 2 hours at room temperature on an ELISA plate shaker (500 shakes per min.).
4.	After incubation, aspirate samples by use of a plate washing machine, or discard the samples by briskly inverting the frame of wells over a suitable receptacle. Wash the wells once with diluted wash solution (J), and aspirate the wash by use of a plate washing machine or discard the wash by briskly inverting the frame of wells over a suitable receptacle. Tap the inverted wells gently on a clean, dry, absorbent surface to remove excess wash solution (only necessary if washing plate by hand).
5.	Pipette <b>100 µL</b> of reconstituted TSH-Biotin (E) into each well (except blank). Avoid splashing the material out of the wells during addition.
6.	Cover the frame, and incubate at room temperature for 25 minutes without shaking.
7.	Repeat wash step 4.
8.	Pipette <b>100 µL</b> of diluted SA-POD (G) into each well (except blank), cover the frame and incubate at room temperature for 20 minutes without shaking.
9.	After incubation, aspirate samples by use of a plate washing machine, or discard the samples by briskly inverting the frame of wells over a suitable receptacle. Wash the wells twice with diluted wash solution (J) followed by once with pure water (to remove any foam) and tap the inverted wells gently on a clean, dry, absorbent surface to remove excess wash solution (if a plate washing machine is used, the plate can be washed 3 times with diluted wash solution (J) only).
10.	Pipette <b>100 µL</b> of TMB (I) into each well (including blank) and incubate in the dark at room temperature for 30 minutes without shaking.
11.	Pipette <b>50 µL</b> stop solution (K) to each well (including blank) cover the frame and shake for approximately 5 seconds on an ELISA plate shaker. Ensure substrate incubations are the same for each well.

<b>12.</b>	Within 15 minutes, read the absorbance of each well at 450 nm using an ELISA plate reader, blanked against the well containing <b>100 µL</b> of TMB (I) and <b>50 µL</b> stop solution (K) only.
------------	--

## RESULT ANALYSIS


A calibration curve can be established by plotting calibrator concentration on the x-axis (log scale) against the absorbance of the calibrators on the y-axis (linear scale). The TRAb concentrations in patients' sera can then be read off the calibration curve [plotted at RSR as a spline log/lin curve (smoothing factor = 0)]. The negative control can be assigned a value of 0.1 to assist in computer processing of assay results. Other data reduction systems can be used. Results can also be expressed as inhibition (%) of TSH binding calculated using the formula;

$$100 \times \left( 1 - \frac{\text{test sample absorbance at 450nm}}{\text{negative control (D1) absorbance 450nm}} \right)$$

Samples with high TRAb concentrations can be diluted in kit negative control (D1). For example, 20 µL of sample plus 180 µL of negative control to give a 10x dilution. Other dilutions (e.g. 100x) can be prepared from a 10x dilution or otherwise as appropriate. Some sera will not dilute in a linear way and we suggest that the dilution giving a value closest to 50% inhibition is used for calculation of TRAb concentration.

**TYPICAL RESULTS** (example only, not for use in calculation of actual results)

Sample	A450 (minus blank)	%I	IU/L
Control D1	2.00	0	0
C1	1.70	15	1
C2	1.50	25	2
C3	0.65	68	8
C4	0.15	93	40
Control D2	1.26	37	3.5

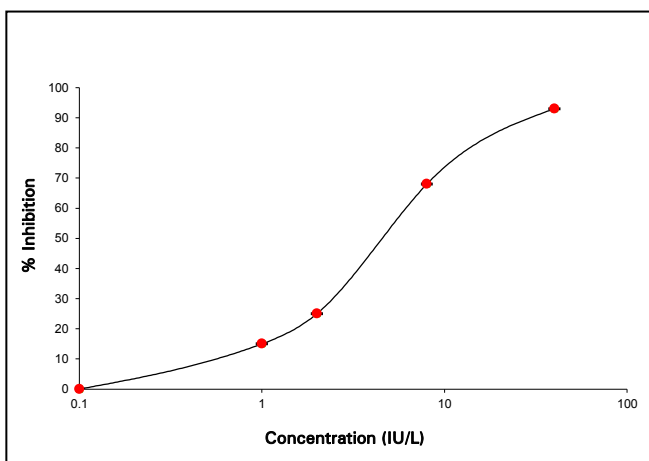

## ASSAY CUT OFF

	IU/L
<b>Negative</b>	≤1 IU/L
<b>Equivocal</b>	1.1 – 1.5 IU/L
<b>Positive</b>	> 1.5 IU/L

This cut off has been validated at RSR. However each laboratory should establish its own normal and pathological reference ranges for TRAb levels. Also it is recommended that each laboratory include its own panel of control samples in the assay.

## CLINICAL EVALUATION

### Clinical Specificity

154 Sera from healthy blood donors were assayed in the RSR TRAb ELISA kit. 152 (99%) were identified as being negative for TRAb.

### Clinical Sensitivity

50 Sera from patients diagnosed with Graves' disease were assayed using the RSR TRAb ELISA kit. 49 (98%) were identified as being positive for TRAb. 1 sample (2%) was identified as being within the equivocal range.

### Functional Sensitivity

A plot of inter assay CV against IU/L indicates a 20% CV occurring at 0.60 IU/L.

### Lower Detection Limit

The kit negative control was assayed 32 times and the mean and standard deviation calculated. The lower detection limit at 2 standard deviations was 0.21 IU/L.

### Inter Assay Precision

Sample	IU/L (n = 20)	CV (%)
1	3.9	12.9
2	5.4	10.9

### Intra Assay Precision

Sample	IU/L (n = 25)	CV (%)
1	1.8	7.1
2	7.8	2.2

### Clinical Accuracy

Analysis of sera from patients with autoimmune diseases other than Graves' disease indicated no interference from autoantibodies to thyroglobulin; thyroid peroxidase; glutamic acid decarboxylase; 21-hydroxylase; acetylcholine receptor; dsDNA or from rheumatoid factor.

### Interference

No interference was observed when samples were spiked with the following materials; haemoglobin at 5 mg/mL; bilirubin at 0.2 mg/mL; Intralipid up to 30 mg/mL, human LH up to 10 u/mL; hCG up to 160 u/mL; human FSH up to 70 u/mL and human TSH up to 3 u/L.

## SAFETY CONSIDERATIONS

### Streptavidin Peroxidase (SA-POD)

Signal word: Warning



#### Hazard statement(s)

H317: May cause an allergic skin reaction

#### Precautionary statement(s)

P280: Wear protective gloves/protective clothing/eye protection/face protection

P302 + P352: IF ON SKIN: Wash with plenty of soap and water

P333 + P313: If skin irritation or rash occurs: Get medical advice/attention

P362 + P364: Take off contaminated clothing and wash it before reuse

### Peroxidase Substrate (TMB)

Signal word: Danger



#### Hazard statement(s)

H360: May damage fertility or the unborn child

#### Precautionary statement(s)

P280: Wear protective gloves/protective clothing/eye protection/face protection

P308 + P313: IF exposed or concerned: Get medical advice/attention

### Diluent for SA-POD and Concentrated Wash Solution

#### Hazard statement(s)

EUH208: Contains 2-Chloroacetamide. May produce an allergic reaction

This kit is intended for *in vitro* use by professional persons only. Follow the instructions carefully. Observe expiry dates stated on the labels and the specified shelf life for coated wells, diluted or reconstituted reagents. Refer to Safety Data Sheet for more detailed safety information. Material of human origin used in the preparation of the kit has been tested and found non-reactive for HIV1 and 2 and HCV antibodies and HBsAg but should, none-the-less, be handled as potentially infectious. Wash hands thoroughly if contamination has occurred and before leaving the laboratory. Sterilise all potentially contaminated waste, including test specimens before disposal. Material of animal origin used in the preparation of the kit has been obtained from animals certified as healthy but these materials should be handled as potentially infectious. Some components contain small quantities of sodium azide as preservative. With all kit components, avoid ingestion, inhalation, injection and contact with skin, eyes and clothing. Avoid formation of heavy metal azides in the drainage system by flushing any kit component away with copious amounts of water.

## ASSAY PLAN

Allow all reagents and samples to reach room temperature (20-25°C) before use.	
Pipette:	<b>75 µL</b> Start buffer into each well (except blank)
Pipette:	<b>75 µL</b> Calibrators (starting with the highest concentration and descending to lowest), controls, patient sera (except blank)
Incubate	2 Hours at room temperature on an <b>ELISA plate shaker at 500 shakes/min</b>
Aspirate/Decant:	Plate
Wash:	Plate once on automatic washer (or wash once, invert and tap dry on absorbent material for manual washing)
Pipette:	<b>100 µL</b> TSH-Biotin (reconstituted) into each well (except blank)
Incubate:	25 Minutes at room temperature <b>without shaking</b>
Aspirate/Decant:	Plate
Wash:	Plate once as above
Pipette:	<b>100 µL</b> SA-POD (diluted 1:20) into each well (except blank)
Incubate:	20 Minutes at room temperature <b>without shaking</b>
Aspirate/Decant:	Plate
Wash:	Plate three times on automatic washer (or wash twice, rinse once with pure water and dry on absorbent material for manual washing)
Pipette:	<b>100 µL</b> TMB into each well (including blank)
Incubate:	30 Minutes at room temperature <b>in the dark without shaking</b>
Pipette:	<b>50 µL</b> Stop solution into each well (including blank) and shake for 5 seconds
Read absorbance at 450 nm, within 15 minutes of adding stop solution	
<b>Do not perform the assay at temperatures above 25 °C.</b>	