



Fast 2 Screen Islet Cell Autoantibody ELISA Kit - Instructions for use 

RSR Limited

Parc Ty Glas, Llanishen,
Cardiff CF14 5DU United Kingdom
Tel.: +44 29 2068 9299 Fax: +44 29 2075 7770
Email: info@rsrltd.com Website: www.rsrltd.com

 Advena Ltd. Tower Business Centre, 2nd Fl.,
Tower Street, Swatar, BKR 4013 Malta.

INTENDED USE

The RSR Fast 2 Screen Islet Cell autoantibody (2 Screen) ELISA kit is intended for use by professional persons only, for quantitative determination of both GAD and IA-2 autoantibodies in human serum.

Autoantibodies to pancreatic beta cell antigens are important serological markers of type 1 diabetes mellitus. The antigens recognised by these antibodies include insulin, glutamic acid decarboxylase (GAD₆₅ kDa isoform), the islet cell antigen named IA-2 or ICA-512 and zinc transporter 8 (ZnT8). RSR's Fast 2 Screen ELISA allows simultaneous measurement of GAD and IA-2 autoantibodies in the same sample.

REFERENCES

S. Chen et al
Sensitive non-isotopic assays for autoantibodies to IA2 and to a combination of both IA2 and GAD₆₅.
Clinica Chimica Acta 2005 357: 74-83
C. Törn et al
Diabetes Antibody Standardization Program: evaluation of assays for autoantibodies to glutamic acid decarboxylase and islet antigen-2.
Diabetologia 2008 51:846-852.

PATENTS

The following patents apply:
US patents US 8,129,132 B2 and US 10,481,156 B2.

ASSAY PRINCIPLE

In RSR's Fast 2 Screen ELISA, GAD and IA-2 autoantibodies (Ab) in patient sera, calibrators and controls are allowed to interact with GAD₆₅ and IA-2 coated onto ELISA plate wells (1st incubation). The samples are then discarded, leaving any GAD or IA-2 autoantibodies in the patient sera, calibrators or controls bound to the GAD₆₅ and IA-2 coated wells. A mixture of GAD₆₅-Biotin and IA-2-Biotin is then added and during a second incubation step (through the ability of GAD and IA-2 autoantibodies to act divalently), a bridge is formed between the GAD₆₅ or IA-2 bound to the wells and GAD₆₅-Biotin or IA-2-Biotin respectively. The amount of GAD₆₅/IA-2-Biotin bound is determined in a third incubation











step by the addition of Streptavidin Peroxidase (SA-POD), which binds specifically to Biotin. Excess unbound SA-POD is then washed away and addition of 3,3',5,5' tetramethylbenzidine (TMB) results in formation of a blue colour. This reaction is stopped by addition of stop solution causing the well contents to turn from blue to yellow. The absorbance of the yellow reaction mixture at 450nm is then read using an ELISA plate reader. A higher absorbance indicates the presence of GAD or IA-2 Ab in the test sample. Reading at 405nm allows quantitation of high absorbances.

This Fast 2 Screen ELISA kit assay is performed in about 4 hours and without refrigeration. It may be particularly suitable for users with automated ELISA processors.

STORAGE AND PREPARATION OF TEST SERUM SAMPLES

Sera to be analysed should be assayed soon after separation or stored, preferably in aliquots, at or below -20°C. 100µL is sufficient for one assay (duplicate 50µL determinations). Repeated freeze thawing or increases in storage temperature must be avoided. Do not use lipaemic or haemolysed serum samples. Do not use plasma in the assay. When required, thaw test sera at room temperature and mix gently to ensure homogeneity. Centrifuge serum prior to assay (preferably for 5 min at 10-15,000 rpm in a microfuge) to remove particulate matter. Please do not omit this centrifugation step if sera are cloudy or contain particulates.

SYMBOLS

Symbol	Meaning
	EC Declaration of Conformity
	In Vitro Diagnostic Device
	Catalogue Number
	Lot Number
	Consult Instructions
	Manufactured By
	Expiry Date
	Store
	Positive Control
	Negative Control

MATERIALS REQUIRED AND NOT SUPPLIED

Pipettes capable of dispensing 25µL, 50 µL and 100µL.

Means of measuring out various volumes to reconstitute or dilute reagents supplied.

Pure water

ELISA Plate reader suitable for 96 well formats and capable of measuring at 450nm and 405nm

ELISA Plate shaker, capable of 500 shakes/min (not an orbital shaker).

ELISA Plate cover

PREPARATION OF REAGENTS SUPPLIED

Store unopened kit and components at 2 - 8°C

A	GAD₆₅ and IA-2 Coated Wells 12 breakapart strips of 8 wells (96 in total) in a frame and sealed in foil bag. Allow to stand at room temperature (20 – 25°C) for at least 30 minutes before opening.
	Ensure stripwells are firmly fitted into frame provided. After opening return any unused wells to the original foil packet with desiccant provided and seal with adhesive tape. Place foil bag in the self-seal plastic bag and store at 2-8°C for up to 8 months.
B	Reaction Enhancer 4 mL coloured red Ready for use
C1-6	Calibrators 4, 10, 20, 70, 145 and 450 u/mL (units are NIBSC 97/550) 6 x 0.7 mL Ready for use
D1	GAD Ab Positive Control 0.7 mL Ready for use
D2	IA-2 Ab Positive Control 0.7 mL Ready for use
D3	Negative Control 0.7 mL Ready for use
E	GAD₆₅/IA-2-Biotin (GAD₆₅ Biotin plus IA-2 Biotin) 3 vials lyophilised
	Reconstitute each vial with the amount of reconstitution buffer for GAD ₆₅ /IA-2-Biotin (F) shown on the vial label. When more than one vial is used, pool the reconstituted vials and mix gently before use. Use on day of reconstitution.
F	Reconstitution Buffer for GAD₆₅/IA-2-Biotin 2 x 15 mL coloured blue Ready for use
G	Streptavidin Peroxidase (SA-POD) 1 x 0.7 mL Concentrated
	Dilute 1 in 20 with diluent for SA-POD (H). For example, 0.5mL (G) + 9.5mL (H). Store at 2 – 8°C for up to 18 weeks after dilution.
H	Diluent for SA-POD 15 mL Ready for use

I	Peroxidase Substrate (TMB) 15 mL Ready for use
J	Concentrated Wash Solution 125 mL Concentrated
	Dilute 10 X with pure water before use. Store at 2 – 8°C up to kit expiry.
K	Stop Solution 12 mL Ready for use

ASSAY PROCEDURE

Allow all reagents to stand at room temperature (20 – 25°C) for at least 30 minutes before use. A repeating Eppendorf type pipette is recommended for steps 2, 6, 9, 11 and 12.

1.	Pipette 50 µL of patient sera, calibrators (C1-6) and controls (D1, D2 and D3) into respective wells in duplicate, leaving one well empty for blank (see step 13).
2.	Pipette 25 µL of reaction enhancer (B) into each well (except blank).
3.	Cover the frame and incubate at room temperature for 2 hours on an ELISA plate shaker (500 shakes per min).
4.	Use an ELISA plate washer to aspirate and wash the wells three times with diluted wash solution (J). If a plate washer is not available, discard the well contents by briskly inverting the frame of wells over a suitable receptacle, wash three times manually and finally tap the inverted wells gently on a clean dry absorbent surface.
5.	Pipette 100µL of reconstituted GAD ₆₅ /IA-2-Biotin (E) into each well (except blank). Avoid splashing the material out of the wells during addition.
6.	Cover the frame and incubate at room temperature for 1 hour on an ELISA plate shaker (500 shakes per min).
7.	Repeat wash step 5.
8.	Pipette 100µL of diluted SA-POD (G) into each well (except blank) and incubate at room temperature for 20 minutes, on an ELISA plate shaker (500 shakes per min).
9.	After the incubation, wash the wells three times with diluted wash solution (J) as in step 4 (in the case of washing manually, use an additional final wash step with pure water to remove any foam).
10.	Pipette 100µL of TMB (I) into each well (including blank) and incubate in the dark at room temperature for 20 minutes without shaking.
11.	Pipette 100µL stop solution (K) into each well (including blank) and shake the plate for approximately 5 seconds on a plate shaker (500 shakes per min). Ensure substrate incubations are the same for each well.

12. Within 10 minutes read the absorbance of each well at 405nm and then 450nm using an ELISA plate reader, blanked against a well containing 100µL of TMB substrate (I) and 100µL Stop solution (K) only.


RESULT ANALYSIS

A calibration curve can be established by plotting calibrator concentration on the x-axis (log scale) against the absorbance of the calibrators on the y-axis (linear scale). The GAD and/or IA-2 Ab concentrations in patient sera can then be read off the calibration curve [Plotted at RSR as a spline log/lin curve (smoothing factor = 0)]. Other data reduction methods can be used. The negative control (D3) has a concentration of 0 u/mL, but can be assigned a value of 0.4 u/mL to facilitate computer processing of data. Absorbance readings at 405nm can be converted to 450nm absorbance values by multiplying by the appropriate factor (approximately 3.4, dependant on equipment being used). Values less than 25 u/mL should be read off a 450 nm curve.

Samples with high GADAb and IA-2 Ab concentrations can be diluted in kit negative control (D3). For example, 15 µL of sample plus 135 µL of negative control to give a 10x dilution. Other dilutions (e.g. 100x) can be prepared from a 10x dilution or otherwise as appropriate. Some sera will not dilute in a linear way.

TYPICAL RESULTS (Example only; not to be used for calculation of actual results)

Calibrator	Absorbance	
	450nm	405nm
u/mL		
Negative Control	0.032	0.010
4	0.216	0.064
10	0.483	0.144
20	0.843	0.252
70	2.969	0.882
145	5.511	1.621
450	8.208	2.414

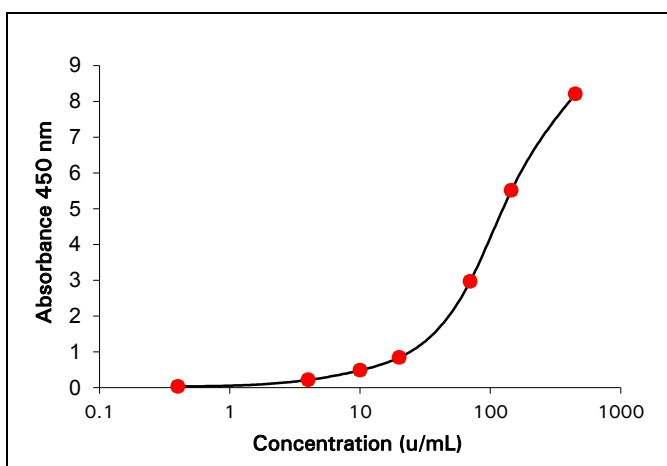

Index Calculation

If results are to be expressed as an index, only the 4 u/mL calibrator need be included in the assay (all controls should still be included). The index values are calculated as follows:

$$\text{Index} = \frac{\text{test sample absorbance at 450nm}}{4 \text{ u/mL calibrator absorbance at 450nm}}$$

Healthy blood donor sera give index values of less than 1 suggesting that index values of 1 or more can be considered positive for GADAb and/or IA-2 Ab.

ASSAY CUT OFF

	u/mL
Negative	< 4.0 u/mL
Positive	≥ 4.0 u/mL

This cut off has been validated at RSR. However each laboratory should establish its own normal and pathological reference ranges for GAD and/or IA-2 Ab levels. Also it is recommended that each laboratory include its own panel of control samples in the assay.

CLINICAL EVALUATION

Clinical Specificity and sensitivity

Sera from 100 individual healthy blood donors were assayed in the Fast 2 Screen ELISA. 99 (99%) were identified as being negative for GAD and/or IA-2 autoantibodies.

Sera from 50 patients diagnosed with Type 1 diabetes were assayed in the Fast 2 Screen ELISA. Autoantibodies to GAD and/or IA2 were detected in 88% (n = 44) of samples.

Limit of Blank and Limit of Detection

The kit negative control and a low analyte sample were assayed 20 times in 3 different kit lots and the mean limit of blank and limit of detection calculated.

Limit of Blank at 2 standard deviations was 0.47 U/mL.

Limit of Detection was 0.68 U/mL.

Intra Assay Precision

Sample	u/mL (n = 25)	CV (%)
1	9.6	14.1
2	17.7	7.9
3	23.2	5.0
4	68.9	3.3
5	309.3	4.4

Inter Assay Precision

Sample	u/mL (n = 20)	CV (%)
1	9.3	8.8
2	19.7	3.5
3	24.9	4.6
4	75.9	4.2
5	360.6	10.8

Clinical Accuracy

Analysis of sera from patients with autoimmune diseases other than type 1 DM indicated no interference from autoantibodies to the TSH receptor (n = 10). One sample positive for rheumatoid factor (n = 20) and one Type 2

Diabetes mellitus patient sera (n=25) were positive for GAD Ab and/or IA2 Ab.

SAFETY CONSIDERATIONS

Streptavidin Peroxidase (SA-POD) and Reaction Enhancer

Signal word: Warning



Hazard statement(s)

H317: May cause an allergic skin reaction

Precautionary statement(s)

P261: Avoid breathing mist, vapours

P272: Contaminated work clothing should not be allowed out of the workplace

P280: Wear protective gloves/protective clothing/eye protection/face protection

P302 + P352: IF ON SKIN: Wash with plenty of soap and water

P333 + P313: If skin irritation or rash occurs: Get medical advice/attention

P362 + P364: Take off contaminated clothing and wash it before reuse

P501: Dispose of contents/container to hazardous or special waste collection point, in accordance with local, regional, national and/or international regulation

Peroxidase Substrate (TMB)

Signal word: Danger



Hazard statement(s)

H360D: May damage the unborn child

Precautionary statement(s)

P202: Do not handle until all safety precautions have been read and understood

P280: Wear protective gloves/protective clothing/eye protection/face protection

P308 + P313: IF exposed or concerned: Get medical advice/attention

P501: Dispose of contents/container to hazardous or special waste collection point, in accordance with local, regional, national and/or international regulation

This kit is intended for *in vitro* use by professional persons only. Follow the instructions carefully. Observe expiry dates stated on the labels and the specified shelf life for coated wells, reconstituted reagents and diluted reagents. Refer to Safety Data Sheet for more detailed safety information. Material of human origin used in the preparation of the kit has been tested and found non reactive for HIV1 and 2 and HCV antibodies and HBsAg but should, none the less, be handled as potentially infectious. Wash hands thoroughly if contamination has occurred and before leaving the laboratory. Sterilise all potentially contaminated waste, including test specimens before disposal. Material of animal origin used in the preparation of the kit has been obtained from animals certified as healthy but these materials should be handled as potentially infectious. Some components contain small quantities of sodium azide as preservative. With all kit components, avoid ingestion, inhalation, injection and contact with skin, eyes and clothing. Avoid formation of heavy metal azides in the drainage system by flushing any kit component away with copious amounts of water.

ASSAY PLAN

Allow all reagents and samples to reach room temperature (20 – 25°C) before use	
Pipette:	50µL Calibrators, Controls, Patient Sera (except blanks)
Pipette:	25µL Reaction Enhancer (except blanks)
Incubate	2 hours at room temperature (20-25°C) on an ELISA plate shaker at 500 shakes/min
Aspirate/Decant:	Plate
Wash:	Plate three times (dry on absorbent material for manual wash)
Pipette:	100µL GAD/IA-2 Biotin (reconstituted) into each well (except blanks)
Incubate:	1 hour at room temperature (20-25°C) on an ELISA plate shaker at 500 shakes/min
Aspirate/Decant:	Plate
Wash:	Plate three times (dry on absorbent material for manual wash)
Pipette:	100µL SAPOD (diluted 1:20) into each well (except blanks)
Incubate:	20 minutes at room temperature (20-25°C) on an ELISA plate shaker at 500 shakes/min
Aspirate/Decant:	Plate
Wash:	Plate three times, (additional rinse with pure water and dry on absorbent material for manual wash)
Pipette:	100µL TMB into each well (including blanks)
Incubate:	20 minutes at room temperature in the dark (without shaking)
Pipette:	100µL stop solution into each well (including blanks) and shake for 5 seconds
Read absorbance at 405nm and 450nm within 10 minutes of stop solution addition.	